

PATENT ABSTRACTS OF JAPAN

(11)Publication number : 08-289885
(43)Date of publication of application : 05.11.1996

(51)Int. Cl. A61B 6/00
A61B 6/00


(21)Application number : 07-098174 (71)Applicant : TOSHIBA CORP
(22)Date of filing : 24.04.1995 (72)Inventor : YAMAMOTO SHUZO

(54) X-RAY DIAGNOSTIC DEVICE

(57)Abstract:

PURPOSE: To position a C arm by one touch operation even when the information of a photographing angle stored beforehand is not memorized.

CONSTITUTION: This X-ray diagnostic device is provided with an automatic positioning function capable of storing the photographing angle of an X-ray image pickup device 214a and an X-ray source 214b arranged so as to hold a testee body therebetween and reproducing the stored photographing angle and a means for displaying the list of the photographing angles stored by the automatic positioning function on a monitor at the time of reproducing the photographing angle.

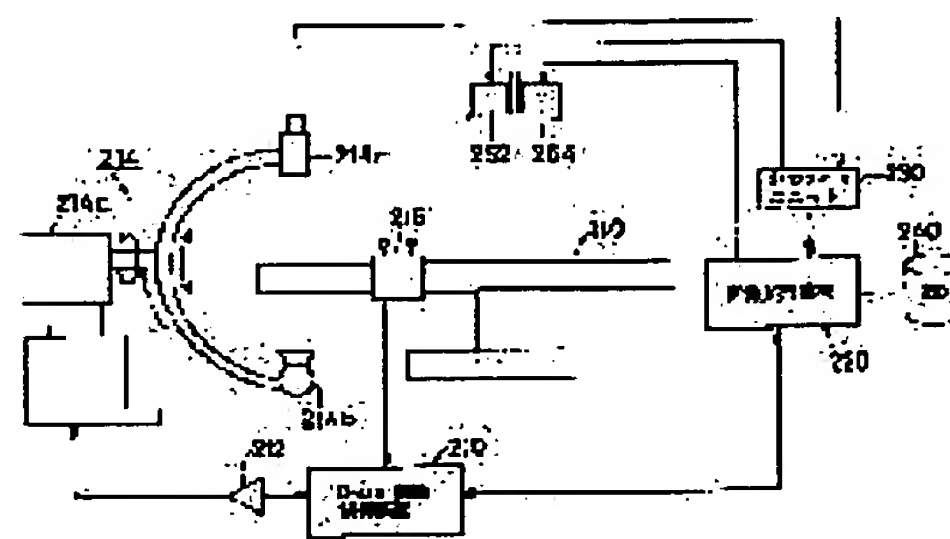

LEGAL STATUS

[Date of request for examination]

[Date of sending the examiner's decision of rejection]

[Kind of final disposal of application other than the examiner's decision of rejection or application converted registration]

[Date of final disposal for application]

[Patent number]

[Date of registration]

[Number of appeal against examiner's decision of rejection]

[Date of requesting appeal against examiner's decision of rejection]

[Date of extinction of right]

Copyright (C); 1998,2000 Japan Patent Office